


## LABSOLUTE® MEASURING CYLINDER, CLASS B low form, with functional spout

### Properties:

- Made of borosilicate glass 3.3
- According to DIN EN ISO 4788
- With functional spout
- Calibrated to „In“ (20 °C) with line graduation
- Labelling with amber diffusion dye
- Solid, hexagonal, glass base
- Dishwasher proof and autoclaveable at 121 °C
- Very high resistance against a wide range of chemicals

### Technical drawing / picture:

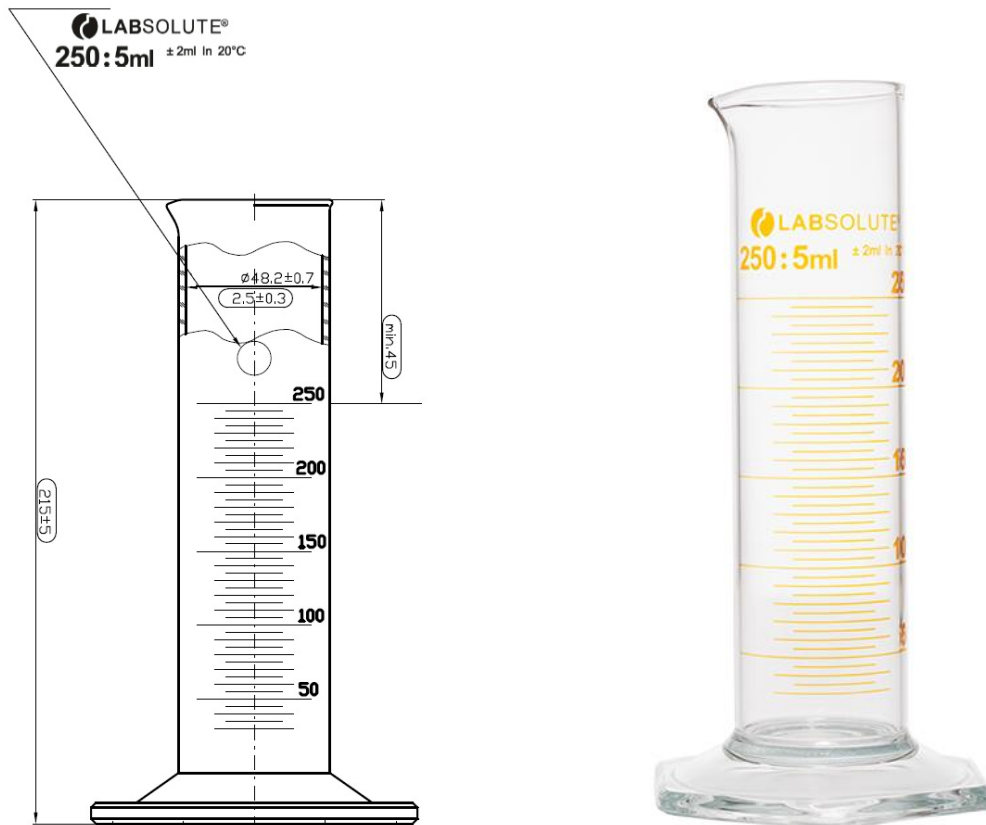

The technical drawing is just an example. Technical drawings of all sizes are available on request.

Th. Geyer GmbH & Co. KG

**Value table:**

Item no.	V ml	Divison ml	Error ± ml	Min ml	Ø1 mm	Ø2 mm	h mm
7.691 010	10	1.0	0.5	2	21.3	53	100
7.691 011	25	1.0	1.0	5	26.0	58	125
7.691 012	50	1.0	1.0	10	31.3	68	150
7.691 013	100	2.0	2.0	12	41.0	85	170
7.691 014	250	5.0	5.0	30	53.2	102	235
7.691 015	500	10.0	10.0	60	67.0	130	280
7.691 016	1,000	20.0	20.0	100	83.5	140	340
7.691 017	2,000	50.0	50.0	100	95.0	150	420

**Description of the abbreviations in the value table:**

Item no.	Item number
V	Nominal volume of the measuring cylinder
Division	Smallest, readable, partial volume
Error	Permitted tolerance for class B acc. to standard (± ml)
Min	Smallest volume of the scale
Ø1	Maximum diameter of the measuring cylinder without spout
Ø2	Diameter of the hexagonal base
h	Maximum height of the measuring cylinder

**Hinweis:**

LABSOLUTE® measuring cylinders are dishwasher-proof. There will be no volume change, if the cylinders are put into a dishwasher at 95 °C and dried in a drying oven at 100 °C afterwards. Please do not use any aggressive cleaning agents, especially ones with very high pH values. The color of the labelling fades away faster using very alkaline cleaning agents. Furthermore those cleaners affect the surface of the measuring cylinder. As a result the calibrated volume can change.

Further information is part of the declaration of conformity.

**Revision 2.0, Stand: 06.07.2018**

**Th. Geyer GmbH & Co. KG**